

Measuring major oral gas components with high precision

OralChroma separates volatile sulfur compounds in oral breath into three major chemicals (hydrogen sulfide, methyl mercaptan, and dimethyl sulfide) and measures their concentration. This feature is greatly helpful to identify halitosis and confirms the treatment effect.

High sensitivity and accuracy

Realize high measurement accuracy with gas chromatograph using our original semiconductor gas sensor and small column.

Easy operation and short measuring time

Measurement automatically starts by simple breath injection and completes in just 4 minutes.

Easy on patients

Short time breath sampling with a small syringe

Maintenance free

Maintenance free for 2 years with a long life sensor and column

Sophisticated data management software attached

Visual halitosis judgment and dental management of each patient history results

OralChroma

Halitosis Measuring Device

Blue: CHM-2-BL Pink: CHM-2-PK

PC is not included.



Specifications

| Product | OralChroma |
|-----------------------|---|
| Detection method | Simple gas chromatography |
| Detection gas | Volatile sulfur compounds 1. Hydrogen sulfide 2. Methyl mercaptan 3. Dimethyl sulfide |
| Operating temperature | 10 to 30°C |
| Storage temperature | -20 to 60°C |
| Power supply | 100 to 240V AC, 50/60Hz |
| Size | 280(W) x 170(H) x 385(D) (mm) |
| External interface | USB |

^{*} Windows are trademarks of Microsoft Corporation in the United States and other countries.

Sample volume 1cc Measuring time 4 minutes ppb and ng/10ml Measuring unit Sampling method Manual sampling with a syringe Operating humidity 80% RH or less (no condensation) Storage humidity 20 to 90% RH (no condensation) Power consumption 60VA Weight 4kg OS for attached software Windows 7 / 8 / 10


Breath measurement view

Two real-time measuring view modes are available. Simple mode (below): Simple bar graph display. Chromatogram mode: Full range chromatogram display.



Measurement history view

Treatment progress and effect can be easily understood with numerical values and graphs. This is useful to explain to patients.

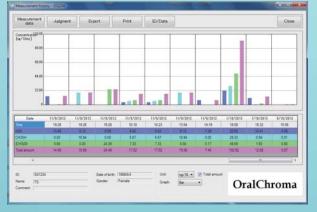

Safety precautions

- Please read the Instruction Manual very carefully before operation.
- Measuring other gases than oral gas may cause malfunction of OralChroma.
- In the interest of continued product improvement, design and specifications may be changed without prior notice.

Nissha FIS, Inc.

2-4-28 Tagawa, Yodogawa-ku, Osaka 532-0027, JAPAN

TEL: +816-7176-3911 FAX: +816-7176-3912

URL: http://www.fisinc.co.jp/en

Contact:

^{*} This product requires a personal computer.

^{*} This product does not include a personal computer.

^{*} This product is a measuring device.